

Chronos

Refraction System

Guided Binocular Refraction.

Streamline your workflow and delegate refraction with Chronos



**COMPACT, RELIABLE REFRACTION
SYSTEM** that combines binocular
autorefractometry and keratometry with
binocular subjective testing and
visual acuity.

Chronos

Refraction System

Streamline your workflow and delegate refraction with Chronos

Chronos is a multifunctional, space-saving instrument
that optimises your workflow.

OVERVIEW



DELEGATE

SightPilot™ is a guided refraction
system that simplifies exams and
facilitates delegation.



STREAMLINE YOUR WORKFLOW

Divert straightforward patients through
Chronos, reserving time for more complex
cases. Customise the Chronos exam
depending on whether it is pre-operative,
post-operative, conventional refraction, etc.



SAVE SPACE

Chronos, as an all-in-one platform
with a small footprint, avoids the
need to factor in the patient-chart
distance in the room layout, saving
space and boosting cost efficiency,
and providing flexibility on where
refraction takes place.



SAVE TIME

Chronos saves time by optimising
the workflow, eliminating the time
needed to clean and move between
devices.

SEE HOW YOU CAN
STREAMLINE YOUR
WORKFLOW AND
DELEGATE REFRACTION
WITH CHRONOS



CHRONOS- ENHANCED WORKFLOW




Time Saving



Maximising
Resource Allocation

Accuracy of refraction is paramount whether you are refracting pre or post-surgery, or undertaking routine refraction. Chronos allows you to delegate refraction without compromise, for straightforward patients.

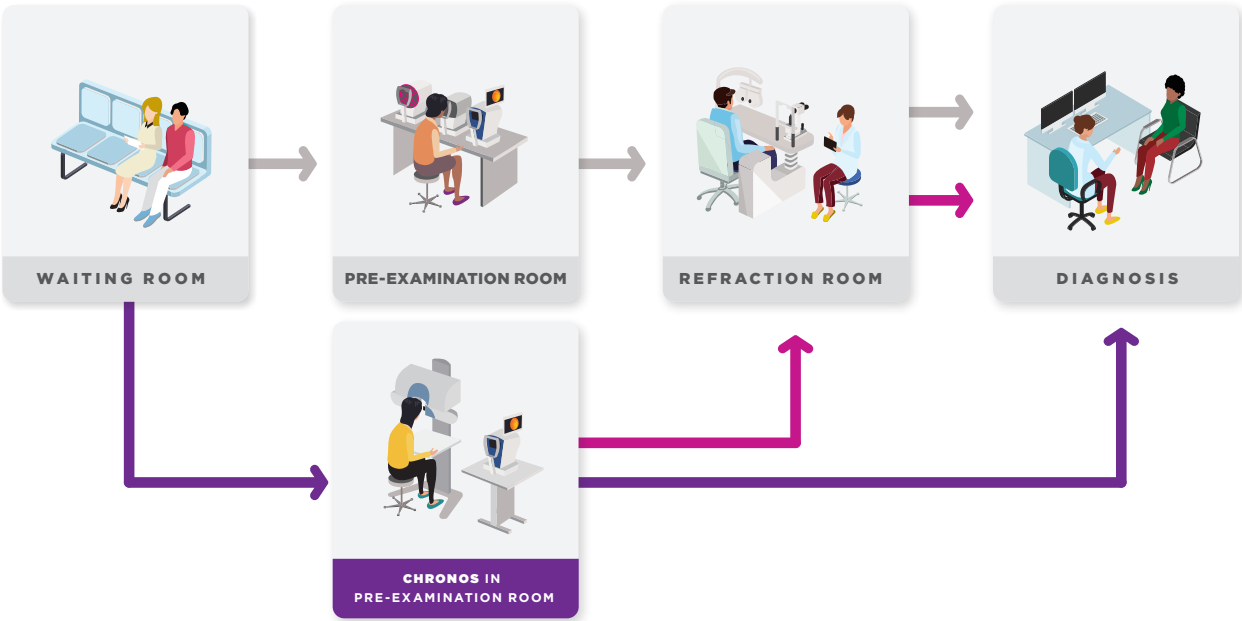

- Current workflow
- Additional pre-operative workflow option by adding Chronos
- Additional post-operative workflow option by adding Chronos

SightPilot™ is optimised for efficient workflow, facilitating delegation

SightPilot™ has a guided user interface which takes you step-by-step through the refraction process. At each step, the operator is given instructions to proceed with the refraction based on the patient's response.



SightPilot Simplify Refraction



- Measurement of Visual Acuity(VA) with previous prescription or unaided¹
- VA screening with binocular objective refraction
- Red/green test
- Cross cylinder
- Binocular balance
- Final monocular and binocular VA with subjective result
- Previous VA vs SightPilot™ VA
- Near test
- Binocular VA at near
- Spherical equivalent vs. full cylinder correction to demonstrate the value of astigmatic correction

1

Patient Details

Enter the patient information and import/enter the previous spectacle prescription to begin the refraction¹.

2

Objective Refraction

SightPilot™ provides step-by-step instructions to position the patient and then automatically aligns the optics to complete the objective refraction.

3

Subjective Refraction

SightPilot™ walks the operator through a variety of subjective refraction tests including visual acuity charts, red-green comparison, cylinder adjustment, binocular balancing and near addition charts. On-screen prompts enable quick input of patient response to advance to the next step in the process.

4

Results

When the refraction is complete, the results are displayed on screen and may be printed or sent to the patient's EHR file.

CHRONOS STANDARD INTERFACE

Chronos can be used as a digital phoropter making use of the standard interface. It offers full customisation of the refraction routine, a wide range of tests including tests to assess binocular status, and the option to create and save one or more refraction routines to suit your preference, or the needs of certain patient groups.

1. Previous prescription can be entered manually or imported directly from your Topcon lensmeter (SOLOS [Handled by VISIA IMAGING S.R.L.] and CL-300)

Chronos


Refraction System

With Chronos **automated binocular refraction system**, spend more time on what matters most, your patients.

Chronos Unique Technology


Chronos binocular refraction technology

Chronos measures both autorefractive and subjective refraction under binocular viewing conditions, for a more natural, comfortable visual experience. Binocular refraction has been shown to provide better control of accommodation for objective and subjective end points.

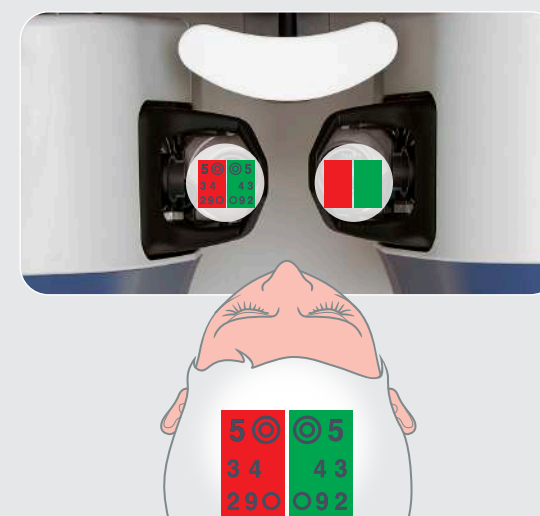

Reduce alignment errors with Chronos auto-alignment

Chronos uses Topcon's 3D stereo camera technology to optimise alignment throughout testing, pioneered in Topcon's automated OCTs and retinal cameras.

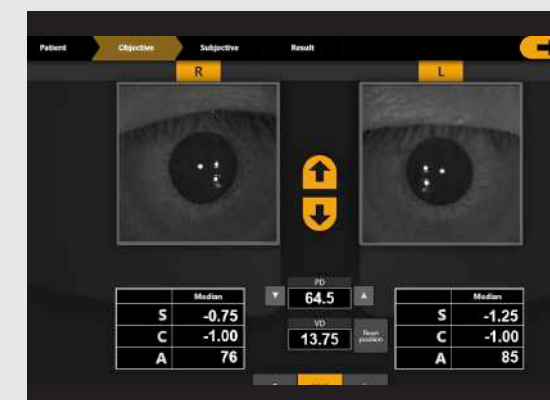

Cutting-edge moving lens system

Chronos incorporates a cutting-edge moving lens system enabling rapid and smooth changes in spherical lens power. This provides a more comfortable visual experience for the patient.




Ease of test distance adjustment

A combination of the built-in θ movement mechanism of the head and the lens movement, adjusts the convergence angle and adjusts the different testing distances.

TEST DISTANCE

Far-/Near-point test distance can be set
25cm - 609.6cm

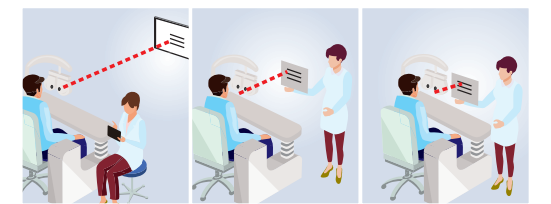


*Conventional refraction set-up, for comparison

Accuracy with Chronos


A combination of the super luminescent diode (SLD) ring, rotary prism technology and binocular objective refraction, provides stable measurements, including in patients with some media opacification.



Measured simultaneously

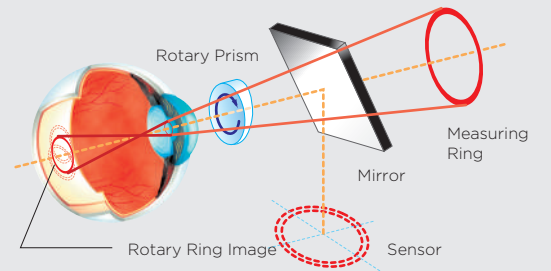

Patented Rotary Prism Technology

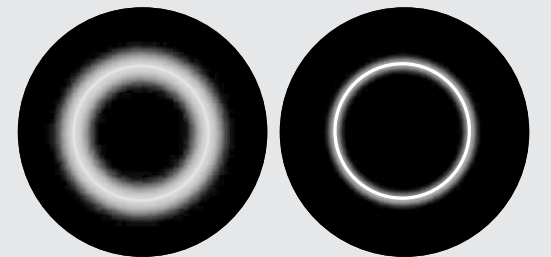

Conventional ring

Chronos ring

Objective measurement

Refraction measurement range	Spherical refractive power	-25D ~ +22D ^{*1,2}
	Cylindrical refractive power	-10D ~ 0D ^{*1,2}
	Cylinder axis angle	1° ~ 180°
Corneal curvature measurement range	Corneal curvature radius	5.00mm ~ 10.00mm
	Corneal refractive power	67.50D ~ 33.75D (Conversion value when the corneal refractive ratio is 1.3375)
	Corneal principal meridian angle	1° ~ 180°
Minimum measurement unit	Spherical/cylindrical refractive power	0.12D
	Cylinder axis angle	1°
	Corneal curvature radius	0.01mm
	Corneal refractive power	0.12D
	Corneal principal meridian angle	1°

Display of measured value	Displayed on the control screen of the operation controller
Minimum measurable pupil diameter	Φ2.0mm
PD measurement range	50mm ~ 80mm
Minimum PD measurement unit	0.5mm

Subjective measurement

Refraction measurement range	Spherical refractive power	-18.00D ≤ Equivalent spherical power ≤ +18.00D ^{*3}
	Cylindrical refractive power	-8.00D ≤ Cylindrical refractive power (Cylindrical power) ≤ 0.00D ^{*4}
	<i>All conditions stated on the right must be met⁵</i>	
	Cylinder axis angle	1° ~ 180°
	Horizontal prism (one eye movable range)	±15.0Δ ^{*6}
	Vertical prism (one eye movable range)	±2.5Δ

Minimum measurement unit	Spherical/ADD refractive power	0.25D
	Cylindrical refractive power	0.25D
	Cylinder axis angle	1°
	Prism refractive power	0.1Δ

Test distance	Far-/Near-point test distance can be set between 25cm and 6.096m
Visual acuity measurement range ⁷	0.05 ~ 1.6 (decimal notation)

Chart	Visual acuity test chart, spherical power correction test chart, astigmatism test chart and binocular function test chart
Background luminance	155±15cd/m²
Display of measured value	Displayed on the screen of the operation controller
Record of measured value	Printing by thermal printer/external printer, data output

Measuring head movement	Right-and-left direction	Inside 9mm to Outside 12.5mm
	Up-and-down direction	Down 15mm to Up 15mm
	Back-and-forth direction	Forward: 20mm - Backward: 20mm
Measuring head rotary angle	Convergence 17.5° to Divergence 8.5° (Eyeball torsion axis centre)	

Other Specifications

Dimensions and Weight	Main unit	Dimensions: 510-540mm (H) × 671-766mm (W) × 278-357mm (D)
	Weight:	31.2 kg
Electric Rating	Power supply unit	Dimensions: 276mm (H) x 117mm (W) x 197mm (D) Weight: 3.5 kg
	Source voltage	AC100 - 240V
	Frequency	50 - 60Hz
	Power input	160VA

^{*1} The dioptric powers are indicated with reference wavelength $\lambda_0 = 587.56 \text{ nm}$
^{*2} Spherical refractive power + Cylindrical refractive power ≤ +22D or Spherical refractive power + Cylindrical refractive power ≥ -25D
^{*3} The conversion value with "VD=12mm" is described here.
^{*4} The conversion value with "VD=-3mm" is described here.
^{*5} The value described here is the maximum value. The measurement range is smaller according to the test distance setting for executing a test or the setting conditions of VD during measurement.
^{*6} The value described here is the maximum value. The measurable range is smaller according to the combination of the patient's PD and the test distance.
^{*7} 0.1 ~ 1.6 complies with ISO 10938. ETDRS chart using Landolt Ring (visual acuity 0.25 ~ 1.6) complies with ANSI Z80.21.



CRX-1000

Chronos Chinrest

For more stable measurement,
an optional chinrest attachment is available.

* This product is in conformity with Regulation EU 2017/745
on medical devices (MDR), Class I.

TOPCON CORPORATION

75-1 Hasunuma-cho, Itabashi-ku, Tokyo 174-8580, JAPAN.
Phone: +81-(0)3-3558-2522/2502 Fax: +81-(0)3-3965-6898
www.topconhealthcare.jp



TOPCON HEALTHCARE SOLUTIONS EMEA OY
Saaristonkatu 9, 90100 Oulu, FINLAND
Phone: +358-0-734-8190
E-mail: thsema.sales@topcon.com
www.topconhealthcare.eu

TOPCON SCANDINAVIA
Neogatan 2, P.O.Box 25, 43151 Mölndal
SWEDEN
Phone: +46-(0)31-7109200
Fax: +46-(0)31-7109249
E-mail: info.hcs.se@topcon.com
www.topconhealthcare.eu/sv_SE

TOPCON FRANCE MEDICAL
1 rue des Vergers, Parc Swen,
Bâtiment 2, 69760 Limonest, FRANCE
Phone: +33-(0)4-37 58 19 40
Fax: +33-(0)4-72 23 86 60
E-mail: topconfrance@topcon.com
www.topconhealthcare.eu/fr_FR

TOPCON GREAT BRITAIN MEDICAL
Topcon House, Kennet Side, Bone Lane,
Newbury, Berkshire RG14 5PX
UNITED KINGDOM
Phone: +44-(0)1635-551120
Fax: +44-(0)1635-551170
E-mail: medical.tgbm@topcon.com
www.topconhealthcare.eu/en_UK

TOPCON EUROPE MEDICAL B.V.
Essebaan 11, 2908 LJ Capelle a/d IJssel
P.O. Box 145, 2900 AC Capelle a/d IJssel
THE NETHERLANDS
Phone: +31-(0)10-4585077
Fax: +31-(0)10-4585045
E-mail: medical@topcon.com
www.topconhealthcare.eu

TOPCON ESPAÑA
Oficina Principal en España
Frederic Mompou, 4,
08960 Sant Just Desvern, Barcelona, SPAIN
Phone: +34-93-4734057
Fax: +34-93-4733932
E-mail: medica@topcon.com
www.topconhealthcare.eu/es_ES

TOPCON DEUTSCHLAND MEDICAL
Hanns-Martin-Schleyer Strasse 41,
D-47877 Willich, GERMANY
Phone: (+49)2154-885-0
Fax: (+49)2154-885-177
E-mail: info@topcon-medical.de
www.topconhealthcare.eu/de_DE

TOPCON IRELAND MEDICAL
Unit 292, Block G, Blanchardstown,
Corporate Park 2 Ballycoolin
Dublin 15, D15 DX58, IRELAND
Phone: +353-12233280
E-mail: medical.ie@topcon.com
www.topconhealthcare.eu/en_IE

TOPCON DANMARK
Praestemarksvej 25, 4000 Roskilde
DANMARK
Phone: +45-46-327500
Fax: +45-46-327555
E-mail: info.todk@topcon.com
www.topconhealthcare.eu/dk_DK

TOPCON ITALY
Viale dell' Industria 60,
20037 Paderno Dugnano, (MI) ITALY
Phone: +39-02-9186671
E-mail: info_tit@topcon.com
www.topconhealthcare.eu/it_IT

TOPCON POLSKA SP. Z. O. O.
ul. Warszawska 23, 42-470 Siewierz
POLAND
Phone: +48-(0)32-670-50-45
Fax: +48-(0)32-671-34-05
E-mail: info.tpl@topcon.com
www.topconhealthcare.eu/pl_PL

IMPORTANT

In order to obtain the best results with this instrument, please be sure to review all user instructions prior to operation.
Medical device MDD Class Im. Manufacturer: Topcon Corporation.

Not all products, services or offers are approved or offered in every market, and products vary from one country to another.
Contact your local distributor for country-specific information and availability.

©2024 Topcon Corporation | M000105E-3

This product is in conformity with Directive 93/42/EEC on medical devices (MDD).

TOPCON Healthcare